


## Cartridges Designed for a Diverse Range of Needs

### FACE CARTRIDGE



### BODY CARTRIDGE

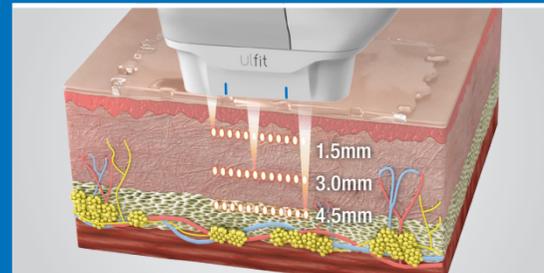

### SYSTEM SPECIFICATIONS

Energy Type	HIFU (High Intensity Focused Ultrasound)
Power	0.1 - 3.0J (0.1J / Step)
Rating	100-240V~, 50/60Hz
Weight	10kg
Dimension	450 (L) X 500 (W) X 270 (H)mm (Including Holders)
Face Cartridge	F7-1.5 (7MHz / 1.5mm) F7-3.0 (7MHz / 3.0mm) F4-4.5 (4MHz / 4.5mm)
Body Cartridge	B2-6.0 (2MHz / 6.0mm) B2-9.0 (2MHz / 9.0mm) B2-13.0 (2MHz / 13.0mm)



UTB06FB2018



CONFIDENTLY FIT with

# ulfit

Ultimate Contouring  
Beyond Expectations

**Cluederm™**  
Entire Beauty Solution

T. +82-2-517-2114 | [cluederm.com](http://cluederm.com) | [info@cluederm.com](mailto:info@cluederm.com)

Images and texts are intellectual property of Cluederm. Copying of this material can be subject to charges of both civil and criminal law of legal justice. Copyright to Cluederm © All Rights Reserved. Export Only

[www.cluederm.com](http://www.cluederm.com)

**Cluederm™**  
Entire Beauty Solution

# Face Lifting & Body Contouring that Satisfies Worldwide

# 317,000+

# ulfit

Advanced Ultrasound of Tomorrow

Engineered to reverse apparent signs of aging powered by MFU and MFCU ultrasound, the ULFIT guarantees non-invasive, comfortable, and customized procedures exclusively on the face, body, or on multiple areas to show the patient's full potential.



## MFU Technology

### Multi-depth Micro Focused Ultrasound

Coupled with slimly designed transducers, the face cartridges of the ULFIT can easily deliver an even distribution of MFU into multiple contours of the face at multiple depths for wrinkle reduction and lifting procedures.




## MFCU Technology

### The Industry's First Macro Focused Circular Ultrasound

The circular design of the multi-depth body cartridges is equipped with MFCU technology that delivers wider coverage as well as equal and precise distribution of high-density ultrasound energy into the focal region.




## Transducer Technology



### Larger Focal Width

Wider transducer yields less pain and precise distribution upon making contact.



### Optional Pain Control

Users may select between "G" (General) and "P" (Pain control) modes to dramatically reduce pain levels.

# 80%

### Reduced Pain

The ULFIT is engineered to deliver treatments with 80% less pain.

# Perfect Treatment for the Body

## Circular Motion Treatment

The ULFIT's body applicator distributes ultrasound energy into large focal regions both evenly and in quick procession.



## Convenient Treatment


- One-Touch Continuous Procedure
- Easy Grip & Lightweight



## Accelerated Shot Speed

The high-peak power capabilities of the body cartridge achieve faster treatment times for equally impressive body outcomes.

88:00 / 100 SHOTS

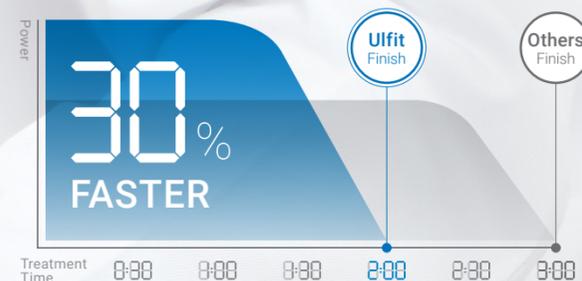

## Application

### FACE

- Forehead
- Periorbital
- Eyebrows
- Wrinkles
- V-line Forming
- Double Chin
- Jowl Lines
- Neck



### BODY

- Axilla
- Arms
- Bra Line
- Abdomen
- Flanks
- Love Handles
- Below Buttocks
- Outer Thighs
- Inner Thighs
- Knees




# Superior Results

## FACE TREATMENT




90% of 20 patients achieved significant facial lifting and tightening outcomes after 1 treatment with the ULFIT.

### Degree of Improvement

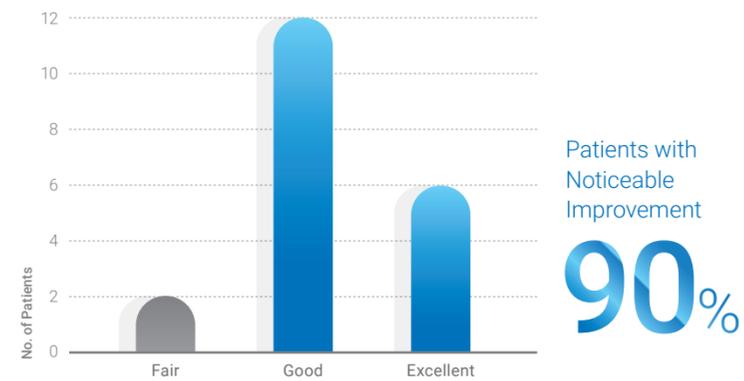


**Target Patients:** 20 individuals in the 20-50 age range with concerns about skin laxity and fine lines and wrinkles on the face. **Testing Period:** 6 weeks. **Testing Methods:** ULFIT 1.5 / 3.0 / 4.5mm Face Cartridges **No. of Treatments:** 1. Both baseline and post treatment measurements of each patient at the 2-week mark were evaluated by three clinicians. **Assessment:** Fair / Good / Excellent.

## BODY TREATMENT

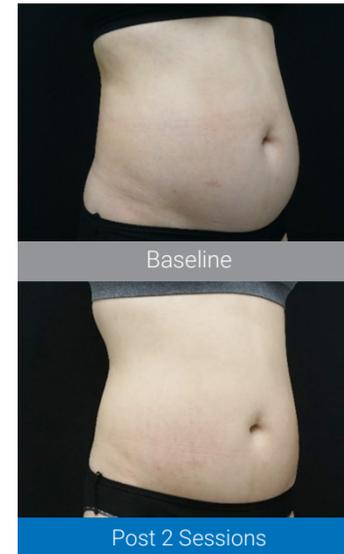


80% of 15 patients achieved a significant reduction of abdominal fat after 1 treatment with the ULFIT.

### Degree of Improvement

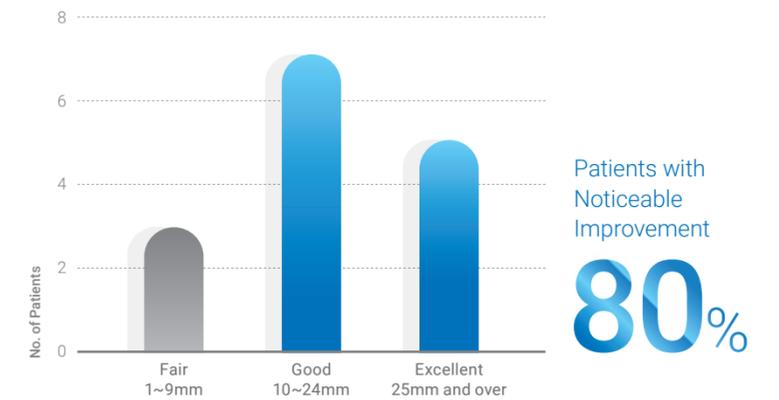


**Target Patients:** 15 individuals in the 20-50 age range with concerns about abdominal circumference. **Testing Period:** 6 weeks. **Testing Methods:** ULFIT 6.0 / 9.0mm Body Cartridges **No. of Treatments:** 1. Both baseline and post treatment measurements of each patient at the 2-week mark were evaluated by three clinicians. **Assessment:** Fair: 1-9mm / Good: 10-24mm / Excellent: 25mm and over.

Age 34 / F

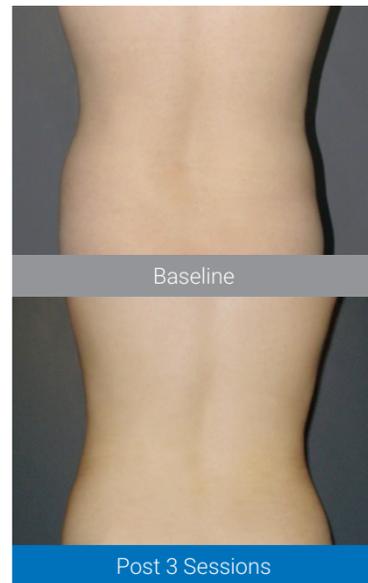


Age 45 / F

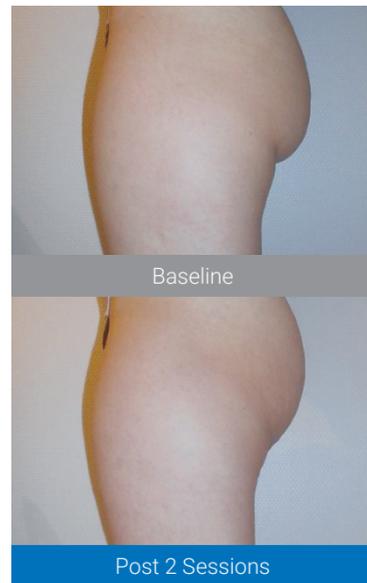

Age 28 / F



Age 38 / F

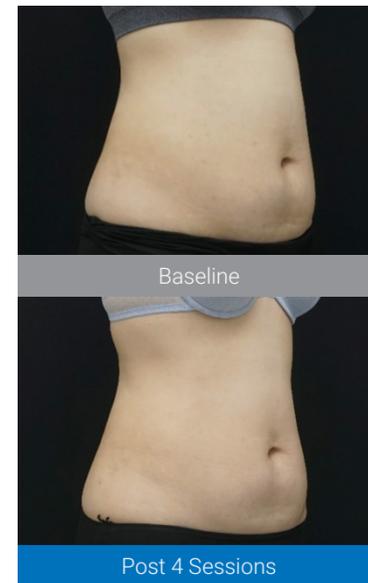

Age 35 / F



Age 35 / F

